



www.nausicaa-medical.com

This device is intended lifts and ceiling-mounted lifts for transferring a person to a sitting position.

It is compatible with lifts equipped with a smooth, open or closed hook system, being able to receive a 40 mm wide sling without impacting the strength of the sling on beams ranging from 2 to 4 points, which excludes hooking with a metal plate with holes.


U ERGONOMIC SLING



- CE certified and manufactured in France, the Ergonomic Sling is recommended for bed / chair / bed transfers and floor pickups when lying down.
- Its U-shaped shape avoids the placement of the strap under the patient's buttocks, making the placement and removal more pleasant for the patient and easier for the caregiver.
- Its back section, combined with the rigid foam headrest, lined with a 3D fabric, increases comfort and protects the spine during transfers.



Before each use, it is important to check: the presence of the label, the stitching of the straps, that they do not fray or come undone, that the device has no tears, snags, holes or signs of fraying (fabric and attachment straps), that the buckles are not cracked or have weak attachments.



The use of the device requires the presence and vigilance of a third person. When used by an agitated or disoriented person, monitoring becomes imperative.

This medical device must be implemented or trained by a health professional.

SMB-PF



v 05.02/23

Important Recommendations :

- In order to get a maximum efficiency of these sort of product, it is necessary :
- to choose the appropriate size for the patient
- to get the best possible adjustment to the patient
- These products must not be in direct contact with a wounded skin.




U ERGONOMIC SLING

SIZES & DIMENSIONS (in cm)

	A	B	C
S	59	88	75
M	65	92	83
L	71	96	92
XL	77	101	102

Composition
100% polyester jersey
3-dimensional polyester fabric
Polyester webbing 40 mm - 1450 DaN
PE foam 50 kg / m³
PE foam 100 kg / m³
40 mm polyester straps
Polyester bias 20 mm

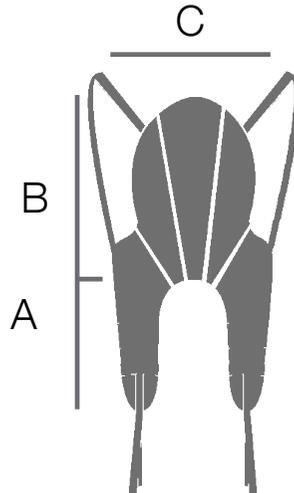

The backrest of this type of strap, is constituted by the wide part of the strap.
The thigh supports, meanwhile, are constituted by the branches of the U.
This type of strap has a system of attachment to the flail of the lifter in four points:

- 2 on both sides of the backsplash,
- 1 at each end of the thigh supports.

Position the bottom of the backrest at the level of the coccyx so that the lines of the attachment system are on both sides of the person. While lifting the person's right leg slightly, move the right thigh support under the right thigh. Proceed in the same way for the left leg. The two leg support systems are located between the legs of the person. Pass these two systems through each other. Hang the two backrest fasteners and the two thigh support attachments to the flail of the mobile lift.

SETTINGS

The hanging system, multiple lines, allows to vary the position of the person.

CAUTION

Read the instructions for use before using the sling.
Hang to the spreader bar the loop which are at the same level.
Do not change any adjustment while the patient is hanging in the sling.
Before lifting a patient, ensure that the sling is correctly hooked on the spreader bar.